


Tracking down smallest biomarkers

November 27 2012

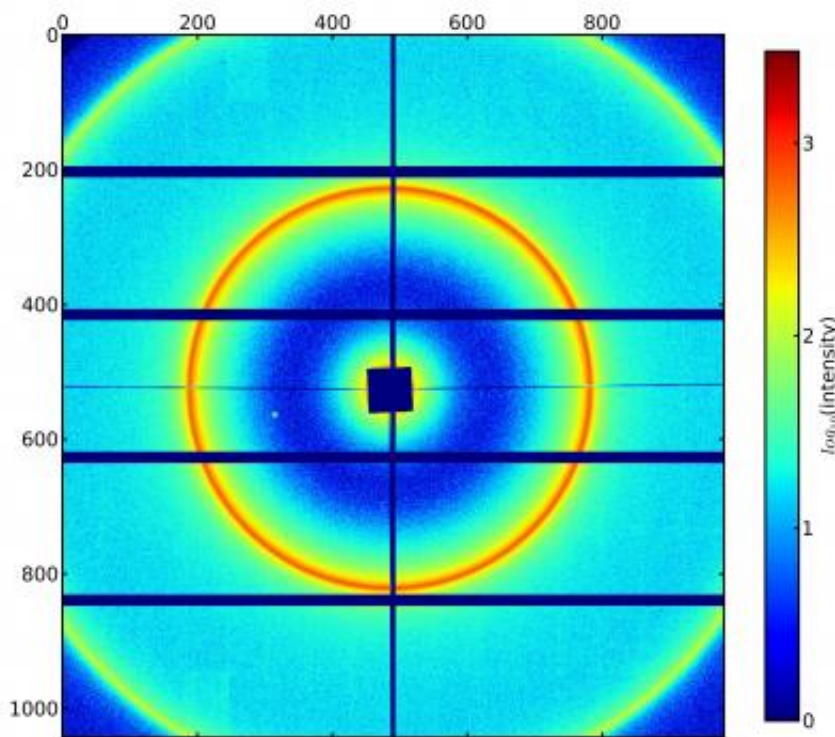

Small-angle X-ray scattering of a micro-vesicle sample (multilamellar liposomes) using the vacuum-compatible Pilatus detector, image recorded at a photon energy of 3 keV. The scattering pattern allows the dimensions of the nano-objects in the examined sample to be determined. Credit: PTB

Microvesicles are smallest cell elements which are present in all body fluids and are different, depending on whether a person is healthy or sick. This could contribute to detecting numerous diseases, such as, e.g., carcinomas, at an early stage, and to treating them more efficiently. The problem is that the diameter of the relevant microvesicles generally lies below 100 nm, which makes them technically detectable, but their exact size and concentration hardly possible to determine.

A new device is now to provide the metrological basis for these promising [biomarkers](#). The vacuum-compatible version of the Pilatus hybrid [pixel detector](#) for X-rays, which was developed by Dectris in cooperation with the Physikalisch-Technische Bundesanstalt (PTB), now allows also the size of nano-particles – which, to date, have been difficult to characterize – to be determined using small-angle X-ray scattering at low photon energies. The detector can also be used for other X-ray-based techniques.

What makes this detector unique is the size of its total surface (17 cm × 18 cm) as well as the fact that it can be operated in vacuum. Operating the detector in vacuum drastically increases the sensitivity of the measuring facility, since the soft X-rays, which are scattered on the sample, are not absorbed by [air molecules](#) on their way towards the detector. This device now allows, for example, experiments for size determination of [nanoparticles](#) to be carried out with small-angle X-ray scattering (SAXS) also at the absorption edges of the [light elements](#) calcium, sulphur, phosphor or silicon at photon energies below 5 keV with high dynamics and good spatial resolution.

For a few months, the new Pilatus X-ray detector has been used for some of PTB's own research projects. At the [synchrotron radiation source](#) BESSY II in Berlin-Adlershof, where PTB has been operating its own laboratory for 15 years, scientists are now using the new detector, for example, to establish the – urgently needed – metrological basis for

the size determination of microvesicles. A project carried out within the scope of the European Metrology Research Programme (EMRP) and with the significant participation of the Amsterdam Medical Center in the Netherlands is to contribute decisively to fully exploiting the potential of microvesicles for the early diagnosis of diseases.

Provided by Physikalisch-Technische Bundesanstalt

Citation: Tracking down smallest biomarkers (2012, November 27) retrieved 2 May 2024 from <https://phys.org/news/2012-11-tracking-smallest-biomarkers.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.