


# Preventing build-up of toxic fouling films on medical devices

February 4 2015

---

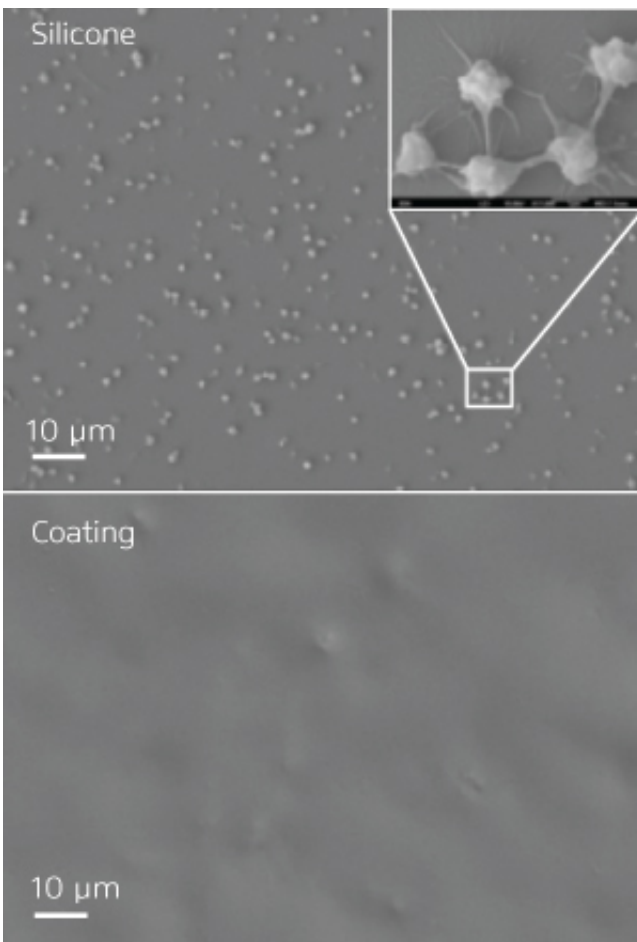

A simple one-step immersion of a catheter surface with brush-like polycarbonates containing pendent adhesive dopamine, antifouling poly(ethylene) glycol and antibacterial cations effectively prevents the fouling of bacteria, protein and platelets with no toxicity. Credit: WILEY-VCH Verlag GmbH & Co. KGaA, Weinheim

A 'one-step' coating that blocks protein growth and kills surface-bound bacteria on silicone may significantly reduce infections from medical devices such as catheters, finds a study led by A\*STAR Institute of Bioengineering and Nanotechnology researchers. Yi Yan Yang and international co-workers accomplished this with a synthetic technique that combines biomimetic surface adhesion and antimicrobial capabilities into a brush-like polymer film.


Implanting foreign materials into biological environments inevitably leads to accumulation, or 'fouling', of surfaces with pathogenic biomolecules. To block this film growth, researchers from the Institute of Bioengineering and Nanotechnology are experimenting with coatings known as '[polymer brushes](#)'—arrays of macromolecular chains that bind to surfaces and modify properties such as bioadhesion.

One popular coating is called poly(ethylene) glycol (PEG), a soft, water-soluble material often used in drug delivery. Chemists can easily modify the structure of PEG for grafting onto device surfaces, where it provides a strong physical barrier against biomolecule adsorption. However, as PEG has no antimicrobial abilities, with time bacteria can overcome the PEG films and grow onto the surface.

Yang and co-workers are working to improve polymer brushes using biodegradable materials called aliphatic polycarbonates. Recently, they developed a 'living' ring-opening polymerization that can attach antimicrobial molecular units and PEG chains to the polycarbonate backbone with high precision. Experiments revealed that catheters coated with this polycarbonate–PEG film eradicated *Staphylococcus* bacteria and had excellent blood compatibility. However, it failed to prevent fouling from one of the most dangerous pathogens in hospitals—*Escherichia coli* bacteria.

Now, the researchers have developed a polymer brush with broad-

spectrum antibacterial capabilities and a simplified coating process. They added three key components to the polycarbonate backbone: effective antimicrobial cations, PEG chains for antifouling, and dopamine groups that stick to silicone rubber in a manner similar to adhesive proteins found in mussel shells. Linking the three components into a single polymer, however, required chemical ingenuity in the form of co-interacting, metal-free catalysts.

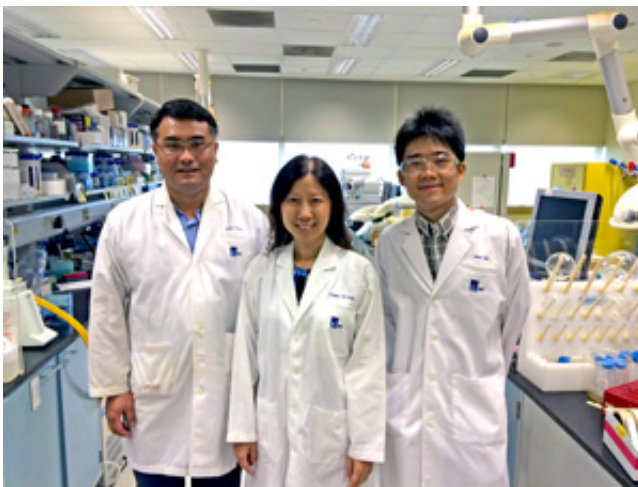

From left to right: Chuan Yang, research scientist, Yi Yan Yang, group leader and Xin Ding, postdoctoral fellow, at the A\*STAR Institute of Bioengineering and Nanotechnology. Credit: A\*STAR Institute of Bioengineering and Nanotechnology

"The amounts of co-catalysts we used were crucial," says Yang. "PEG is a large molecule, and we had to add the catalysts in a stepwise manner to ensure a complete reaction."

The polymer's dopamine groups allowed attachment to catheter surfaces through a single-step dipping procedure. Imaging tests showed that the film killed both *Staphylococcus* and *E. coli* bacteria upon contact, and

prevented these pathogens from establishing fouling layers (see image). Yang notes that these findings, in combination with the coating's stability under simulated blood flow, indicate this approach's potential for preventing infection in intravascular catheters.

**More information:** Yang, C., Ding, X., Ono, R. J., Lee, H., Hsu, L. Y. et al. "Brush-like polycarbonates containing dopamine, cations, and PEG providing a broad-spectrum, antibacterial, and antifouling surface via one-step coating." *Advanced Materials* 26, 7346–7351 (2014).

[dx.doi.org/10.1002/adma.201402059](https://doi.org/10.1002/adma.201402059)

Provided by Agency for Science, Technology and Research (A\*STAR), Singapore

Citation: Preventing build-up of toxic fouling films on medical devices (2015, February 4) retrieved 18 April 2024 from

<https://phys.org/news/2015-02-build-up-toxic-fouling-medical-devices.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.