

Wearable graphene-based biomedical device to monitor and combat diabetes

March 21 2016

Skin-based Diabetes Monitoring and Therapy

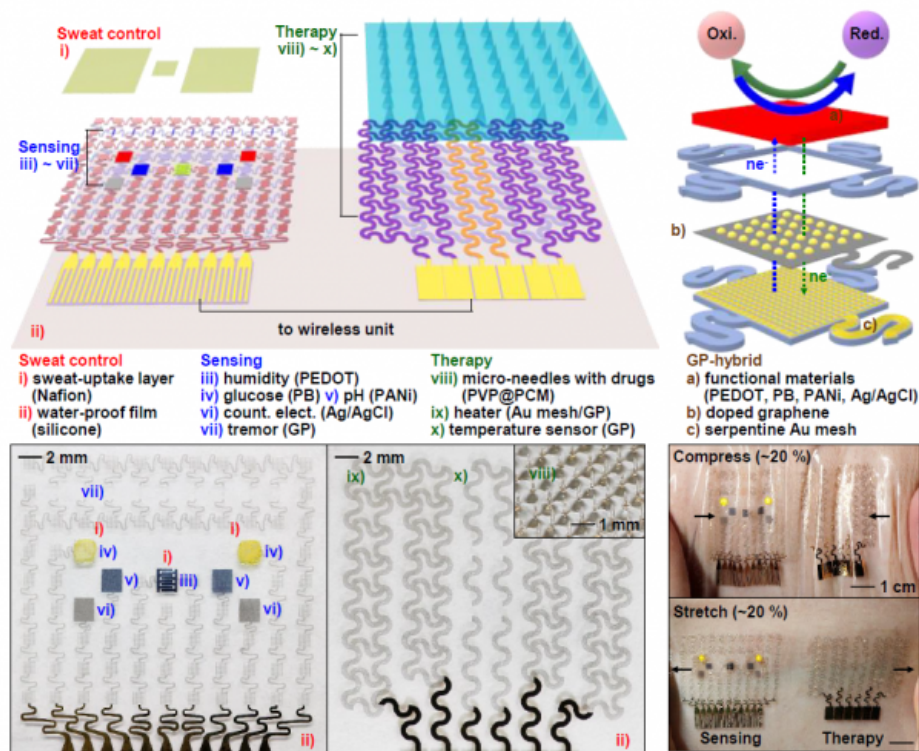


Figure 1. Schematic and corresponding images of the GP-hybrid electrochemical devices and thermoresponsive drug delivery microneedles. Credit: IBS

A scientific team from the Center for Nanoparticle Research at IBS has created a wearable GP-based patch that allows accurate diabetes monitoring and feedback therapy by using human sweat. The researchers improved the device's detecting capabilities by integrating electrochemically active and soft functional materials on the hybrid of gold-doped graphene and a serpentine-shape gold mesh. The device's pH and temperature monitoring functions enable systematic corrections of sweat glucose measurements as the enzyme-based glucose sensor is affected by pH (blood acidity levels) and temperature.

Diabetes and regulating glucose levels

Insulin is produced in the pancreas and regulates the use of glucose, maintaining a balance in blood sugar levels. Diabetes causes an imbalance: insufficient amounts of insulin results in high blood [glucose levels](#), known as hyperglycemia. Type 2 diabetes is the most common form of diabetes with no known cure. It affects some 3 million Koreans with the figure increasing due to dietary patterns and an aging society. The current treatments available to diabetics are painful, inconvenient and costly; regular visits to a doctor and home testing kits are needed to record glucose levels. Patients also have to inject uncomfortable insulin shots to regulate glucose levels. There is a significant need for non-invasive, painless, and stress-free monitoring of important markers of diabetes using multifunctional wearable devices. The IBS [device](#) facilitates this and thereby reduces the lengthy and expensive cycles of visiting doctors and pharmacies.

Components of the graphene-based wearable device

Skin-based Diabetes Monitoring and Therapy

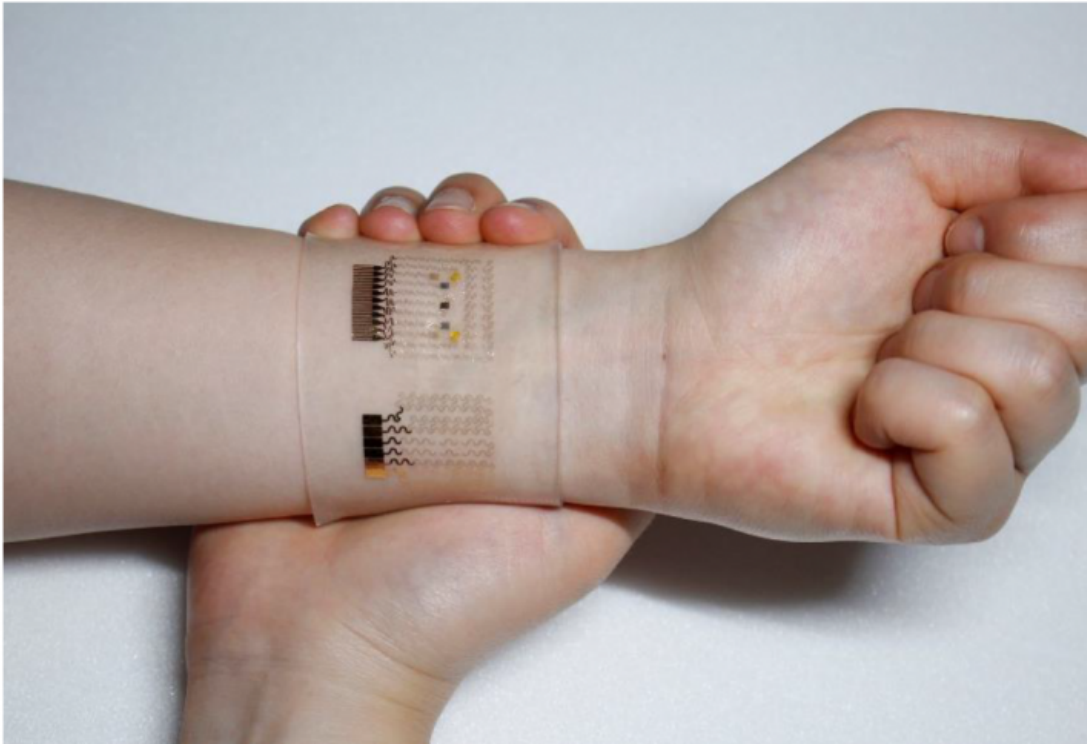


Figure 2. Optical image of the GP-hybrid electrochemical device array on the human skin Credit: IBS

KIM Dae-Hyeong, a scientist from the Center for Nanoparticle Research, describes the vast array of components: "Our wearable GP-based device is capable of not only sweat-based glucose and pH monitoring but also controlled transcutaneous drug delivery through temperature-responsive microneedles. Precise measurement of sweat glucose concentrations are used to estimate the levels of glucose in the blood of a patient. The device retains its original sensitivity after multiple uses, thereby allowing for multiple treatments. The connection

of the device to a portable/ wireless power supply and data transmission unit enables the point-of-care treatment of diabetes." The professor went on to describe how the device works, "The patch is applied to the skin where sweat-based glucose monitoring begins on sweat generation. The humidity sensor monitors the increase in relative humidity (RH). It takes an average of 15 minutes for the sweat-uptake layer of the patch to collect sweat and reach a RH over 80% at which time glucose and pH measurements are initiated."

Merits of the device and drug administration

The device shows dramatic advances over current treatment methods by allowing non-invasive treatments. During the team's research, two healthy males participated in tests to demonstrate the sweat-based glucose sensing of the device. Glucose and pH levels of both subjects were recorded; a statistical analysis confirmed the reliable correlation between sweat glucose data from the diabetes patch and those from commercial glucose tests. If abnormally high levels of glucose are detected, a drug is released into a patient's bloodstream via drug loaded microneedles. The malleable, semi-transparent skin-like appearance of the GP device provides easy and comfortable contact with human skin, allowing the sensors to remain unaffected by any skin deformations. This enables stable sensing and efficient drug delivery.

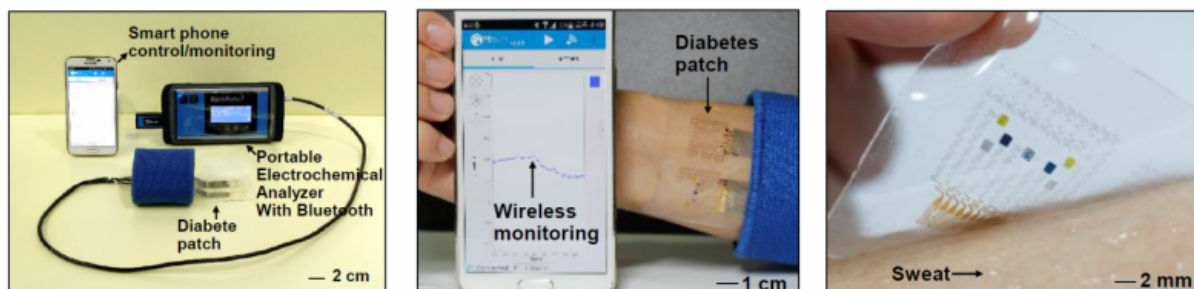


Figure 3. Demonstration of the wearable diabetes monitoring and therapy system in vivo. Credit: IBS

The scientific team also demonstrated the therapeutic effects by experimenting on diabetic (db/db) mice. Treatment began by applying the device near the abdomen of the db mouse. Microneedles pierced the skin of the mouse and released Metformin, an insulin regulating drug, into the bloodstream. The group treated with microneedles showed a significant suppression of blood [glucose](#) concentrations with respect to control groups. "One can easily replace the used microneedles with new ones. Treatment with Metformin through the skin is more efficient than that through the digestive system because the drug is directly introduced into metabolic circulation through the skin," commented KIM Dae-Hyeong. He went on: "These advances using nanomaterials and devices provide new opportunities for the treatment of chronic diseases like diabetes."

More information: Hyunjae Lee et al. A graphene-based electrochemical device with thermoresponsive microneedles for diabetes monitoring and therapy, *Nature Nanotechnology* (2016). [DOI: 10.1038/NNANO.2016.38](https://doi.org/10.1038/NNANO.2016.38)

Provided by Institute for Basic Science

Citation: Wearable graphene-based biomedical device to monitor and combat diabetes (2016, March 21) retrieved 2 May 2024 from <https://phys.org/news/2016-03-wearable-graphene-based-biomedical-device-combat.html>

<p>This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.</p>
--