


# **Researchers create smartphone system to test for lead in water**

September 26 2018, by Jeannie Kever

---

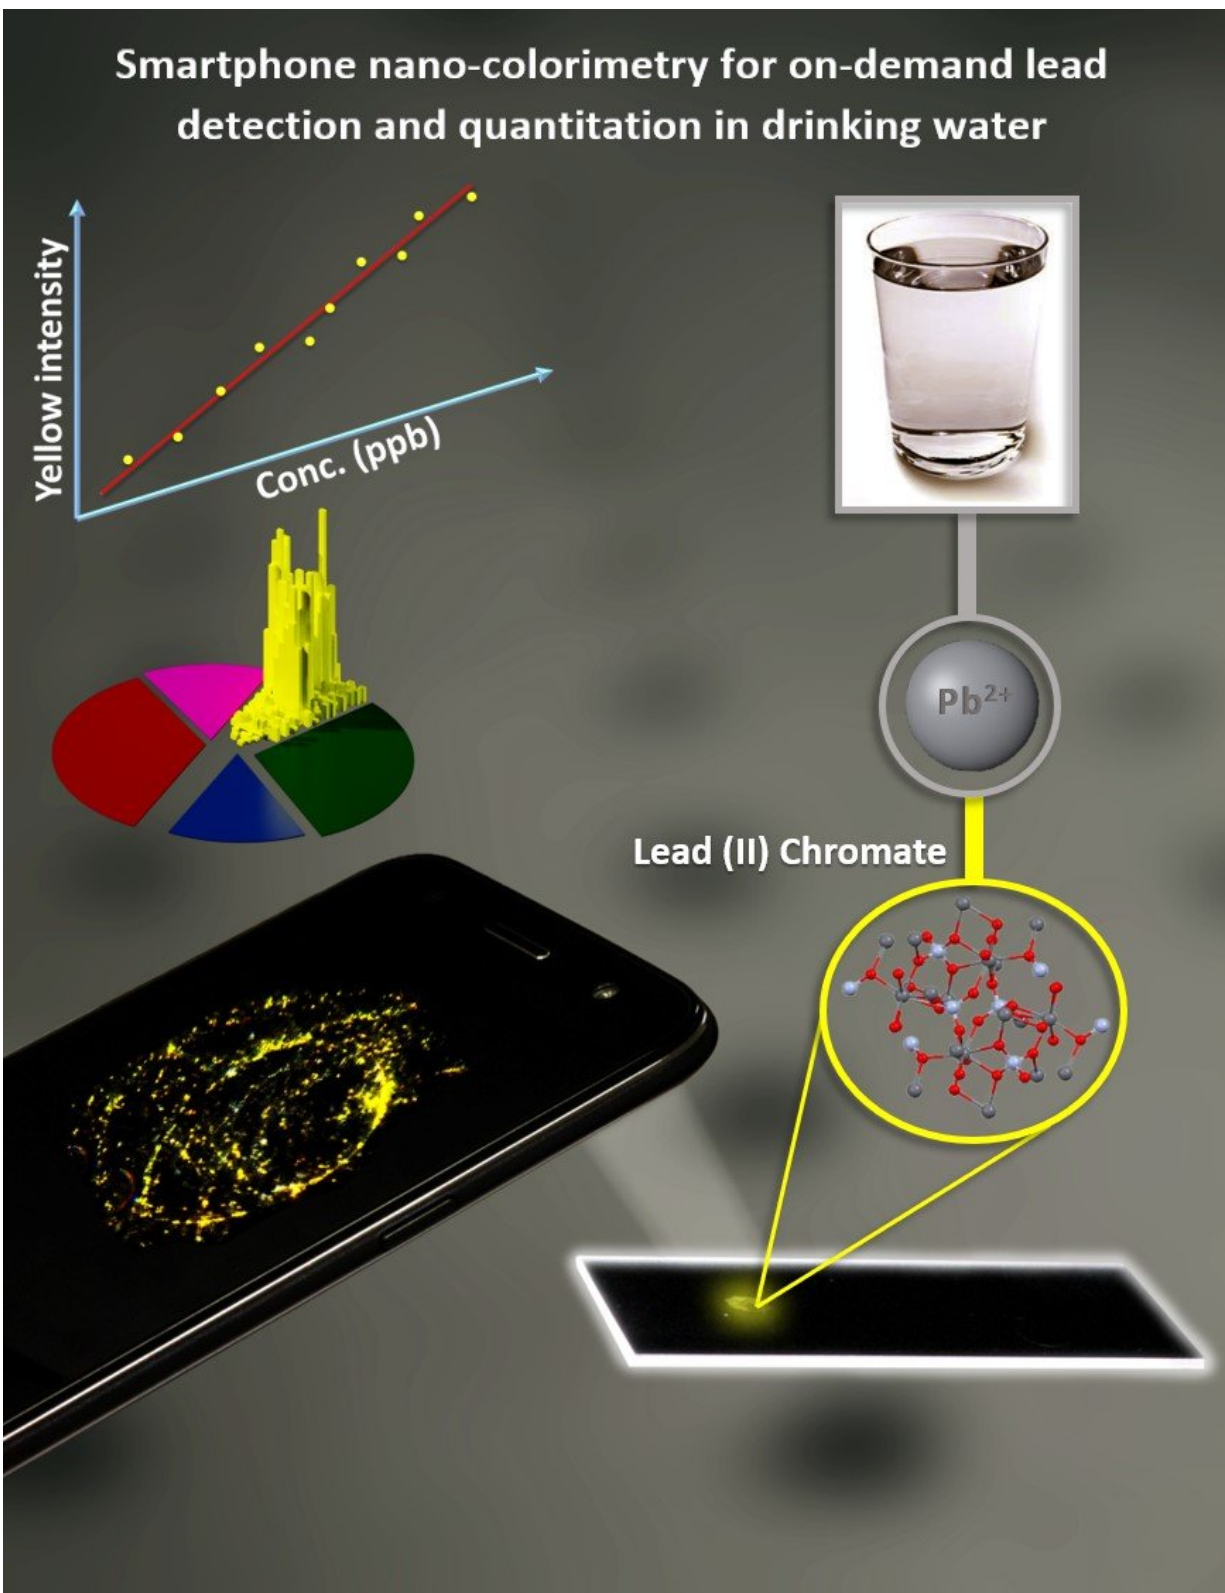

Researchers built a self-contained smartphone microscope that can operate in

both fluorescence and dark-field imaging modes and paired it with an inexpensive Lumina 640 smartphone with an 8-megapixel camera. Credit: University of Houston

The discovery of lead in Flint, Michigan's drinking water drew renewed attention to the health risks posed by the metal. Now researchers at the University of Houston have created an inexpensive system using a smartphone and a lens made with an inkjet printer that can detect lead in tap water at levels commonly accepted as dangerous.

The system builds upon earlier work by Wei-Chuan Shih, associate professor of electrical & computer engineering, and members of his lab, including the [discovery](#) of an inexpensive elastomer lens that can convert a basic [smartphone](#) into a microscope.

The latest discovery, [described](#) in the journal *Analytical Chemistry*, combines nano-colorimetry with dark-field microscopy, integrated into the smartphone microscope platform to detect levels of lead below the safety threshold set by the Environmental Protection Agency.

"Smartphone nano-colorimetry is rapid, low-cost, and has the potential to enable individual citizens to examine (lead) content in [drinking water](#) on-demand in virtually any environmental setting," the researchers wrote.

Even small amounts of lead can cause serious health problems, with young children especially vulnerable to neurological damage. EPA standards require lead levels in drinking [water](#) to be below 15 parts per billion, and Shih said currently available consumer test kits aren't sensitive enough to accurately detect lead at that level.

By using an inexpensive smartphone equipped with an inkjet-printed lens and using the dark-field imaging mode, researchers were able to produce a system that was both portable and easy to operate, as well as able to detect lead concentrations at 5 parts per billion in [tap water](#). The sensitivity reached 1.37 parts per billion in deionized water.

Shih and his students last year [published](#) an open-source dataset in *Biomedical Optics Express*, explaining how to convert a smartphone equipped with the elastomer lens into a microscope capable of fluorescence microscopy. That paper has been the journal's most frequently downloaded paper since its publication.

The latest application incorporates color analysis to detect nanoscale lead particles. In addition to Shih, researchers on the project include first author Hoang Nguyen and Yulung Sung, Kelly O'Shaughnessy and Xiaonan Shan, all with the UH Department of Electrical & Computer Engineering. (O'Shaughnessy was a summer intern from the University of Cincinnati under the National Science Foundation's Research Experiences for Undergraduates program.)

Applying the dataset published in 2017, the researchers built a self-contained smartphone microscope that can operate in both fluorescence and dark-field imaging modes and paired it with an inexpensive Lumina 640 smartphone with an 8-megapixel camera. They spiked tap water with varying amounts of lead, ranging from 1.37 parts per billion to 175 parts per billion. They then added chromate ions, which react with the lead to form lead chromate nanoparticles; the nanoparticles can be detected by combining colorimetric analysis and microscopy.

The analysis measured both the intensity detected from the nanoparticles, correlating that to the lead concentration, and verified that the reaction was spurred by the presence of lead.

The mixture was transferred to a polydimethylsiloxane slab attached to a glass slide; after it dried, deionized water was used to rinse off the chromate compound and the remaining sediment was imaged for analysis.

The microscopy imaging capability proved essential, Shih said, because the quantity of sediment was too small to be imaged with an unassisted smartphone camera, making it impossible to detect relatively low levels of lead.

Building upon the smartphone microscope platform to create a useful consumer product was key, Shih said. "We wanted to be sure we could do something that would be useful from the standpoint of detecting lead at the EPA standard," he said.

**More information:** Hoang Nguyen et al. Smartphone Nanocolorimetry for On-Demand Lead Detection and Quantitation in Drinking Water, *Analytical Chemistry* (2018). [DOI: 10.1021/acs.analchem.8b02808](https://doi.org/10.1021/acs.analchem.8b02808)

Yu-Lung Sung et al. Fabricating optical lenses by inkjet printing and heat-assisted in situ curing of polydimethylsiloxane for smartphone microscopy, *Journal of Biomedical Optics* (2015). [DOI: 10.1117/1.JBO.20.4.047005](https://doi.org/10.1117/1.JBO.20.4.047005)

Provided by University of Houston

Citation: Researchers create smartphone system to test for lead in water (2018, September 26) retrieved 3 May 2024 from <https://phys.org/news/2018-09-smartphone.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is

provided for information purposes only.