


Elastic kirigami patch for electromyographic analysis of the palm muscle during baseball pitching

December 27 2019, by Thamarasee Jeewandara

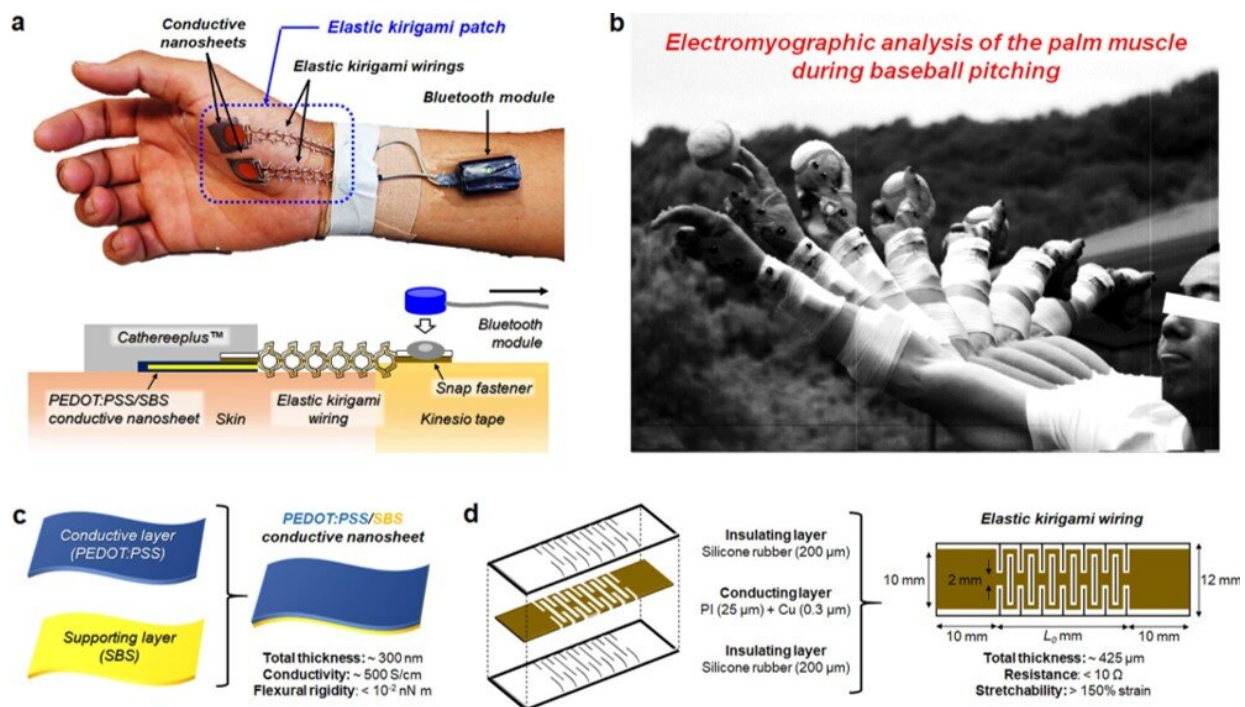


Elastic kirigami patch consisting of conductive nanosheets and elastic kirigami wirings for sEMG recording on the palm muscle during baseball pitching. (a) Image (top) and schematic illustration (bottom) of the elastic kirigami patch attached to the skin and connected to a Bluetooth module. The elastic kirigami patch consists of two conductive nanosheets and two elastic kirigami wirings. (b) Sequential photographs of the pitching motion recorded by high-speed cameras. (c) Schematic illustration of the PEDOT:PSS/SBS conductive nanosheet. (d) Constitution of the elastic kirigami wiring. Credit: Nature Asia Materials, doi: 10.1038/s41427-019-0183-1

Surface electromyography (sEMG) is widely used to investigate human motion including athletic performance. Baseball pitchers require very precise movements to pitch the ball to the strike zone, where the palm muscle plays a key role during movement. Recording the sEMG from the palm can help analyze motion during baseball pitching, however, currently available devices are bulky with rigid electrodes that impede natural movement of the wearer. Kento Yamagishi and a team of researchers in the School of Advanced Science and Engineering, Faculty of Sports, and Digital Manufacture and Design in Japan, therefore described a new skin-contact patch. The wearable device contained kirigami-based stretchable wirings and conductive polymer nanosheet-based ultraconformable bioelectrodes. The research team designed the device to address the mechanical mismatch between human skin and electronics and published the results on *Nature Asia Materials*.

The device contained a kirigami-inspired wiring design and mechanical gradient structure from nanosheet-based flexible bioelectronics to form a bulk wearable construct. The design approach buffered the mechanical stress applied to the skin-contact bioelectrodes during an arm swing movement. More specifically, Yamagishi et al. measured the sEMG at [the abductor pollicis brevis muscle](#) (APBM) in a baseball player during pitching. The research team observed differences in the activity of the APBM between different types of fastball and curveball pitches. The outcomes will allow them to analyze motion in unexplored [muscle](#) areas such as the palm and sole. The work will lead to deeper analysis of muscle activity during a range of sports activities and other movements.

Wearable devices can facilitate accurate measurements of sEMG during exercise via recordings with small electrodes attached to the [skin surface](#) and connected to an amplifier with wires/ However, such devices can restrict vigorous movements. The palm muscle plays a key role for

baseball pitchers, requiring very precise movement within a two-millisecond window to [pitch the ball into the strike zone](#). Since the ball directly touches the palm muscle, obtaining sEMG recordings from the palm during an actual pitch is extremely difficult. Furthermore, if researchers attached electrodes to the palm instead of the palm muscle, it is likely to strain lead wires due to wrist flexes. As a result, researchers had previously restricted sEMG analyses during baseball pitching to [the elbow](#), [scapular muscles](#) and [lower](#) and [upper extremities](#) without examining the palm muscle during ball release.

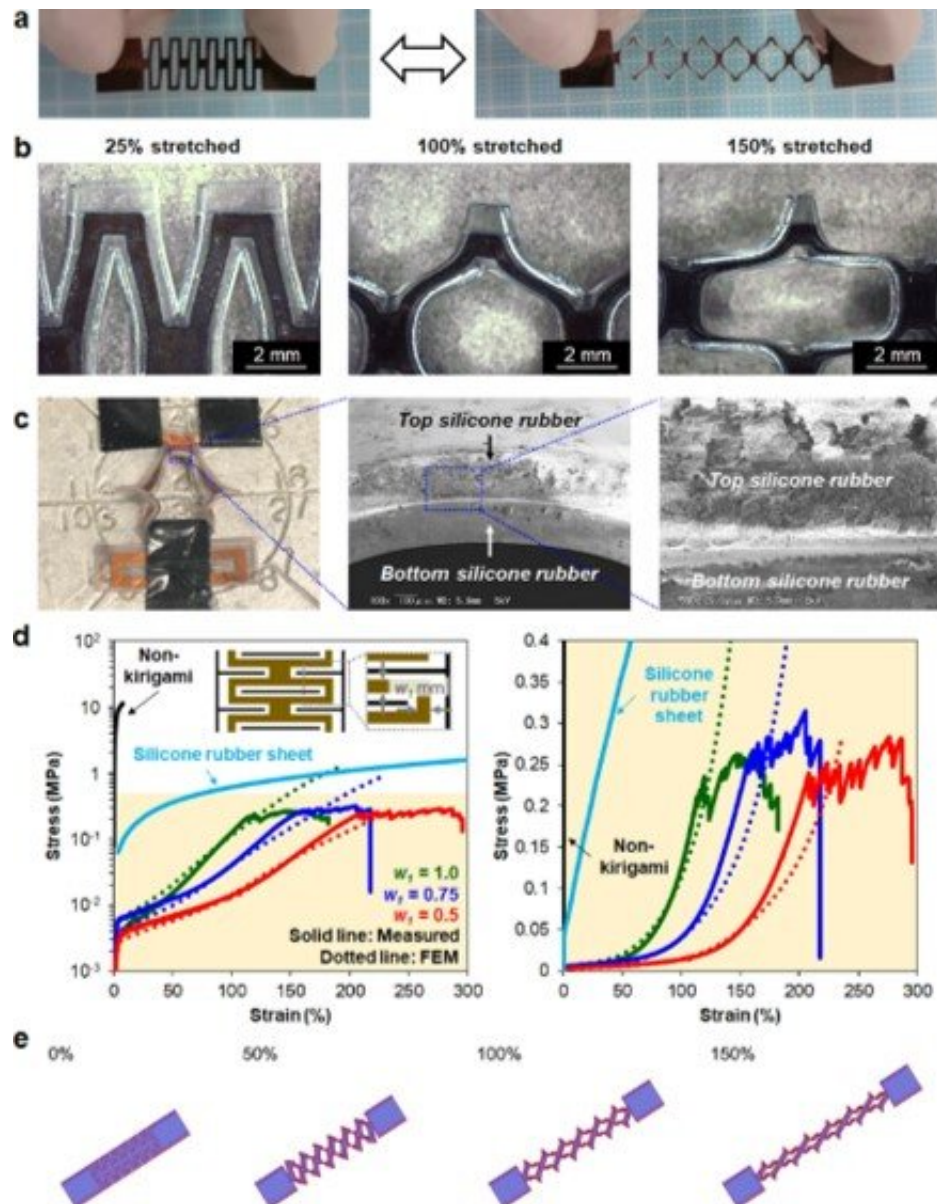


Mechanical properties of elastic kirigami wirings. (a) Images of the elastic kirigami wiring before (left) and after (right) stretching by hand force. (b) Microscopic images of the elastic kirigami wiring elongated at 25% (left), 100% (middle), and 150% (right) strain. (c) Optical (left) and SEM images (middle and right) of the elastic kirigami wiring under 150% strain. There is no delamination between the top and bottom silicone rubber layers. (d) Stress–strain curves of the elastic kirigami wirings of three different designs, the non-kirigami sample, and the silicone rubber sheet (solid lines: measured, dotted lines: FEM-simulated). Left and right graphs are shown in exponential and linear scales of stress, respectively. (e) FEM-simulated images of the elastic kirigami wiring of

$w_1/w_2/w_3/w_4 = 0.75/3.5/0.5/1.0$ at 0%, 50%, 100%, and 150% (from left to right) tensile strain. Credit: Nature Asia Materials, doi: 10.1038/s41427-019-0183-1

In the present work, Yamagishi et al. addressed the problem by developing a skin-contact patch containing conductive polymer nanosheet-based ultraconformable electrodes and "kirigami"-based stretchable wiring. [Kirigami](#) is a type of Japanese paper art widely employed in the field of stretchable electronics due to its flexibility. The technique can render generally unstretchable and rigid two-dimensional (2-D) materials [such as graphene](#) and [carbon-nanotube nanocomposites](#) to be stretchable [via 3-D deformation](#). To connect nanosheet-based bioelectrodes and a bulk wearable mode, Yamagishi et al. designed and developed a kirigami-based wiring system possessing the following features.

1. 2-D-membrane-based conformable skin adhesion
2. Stretchability with minimal changes in resistance, and
3. A fully insulated structure with a conductive layer and kirigami-patterned elastomeric insulating layers.

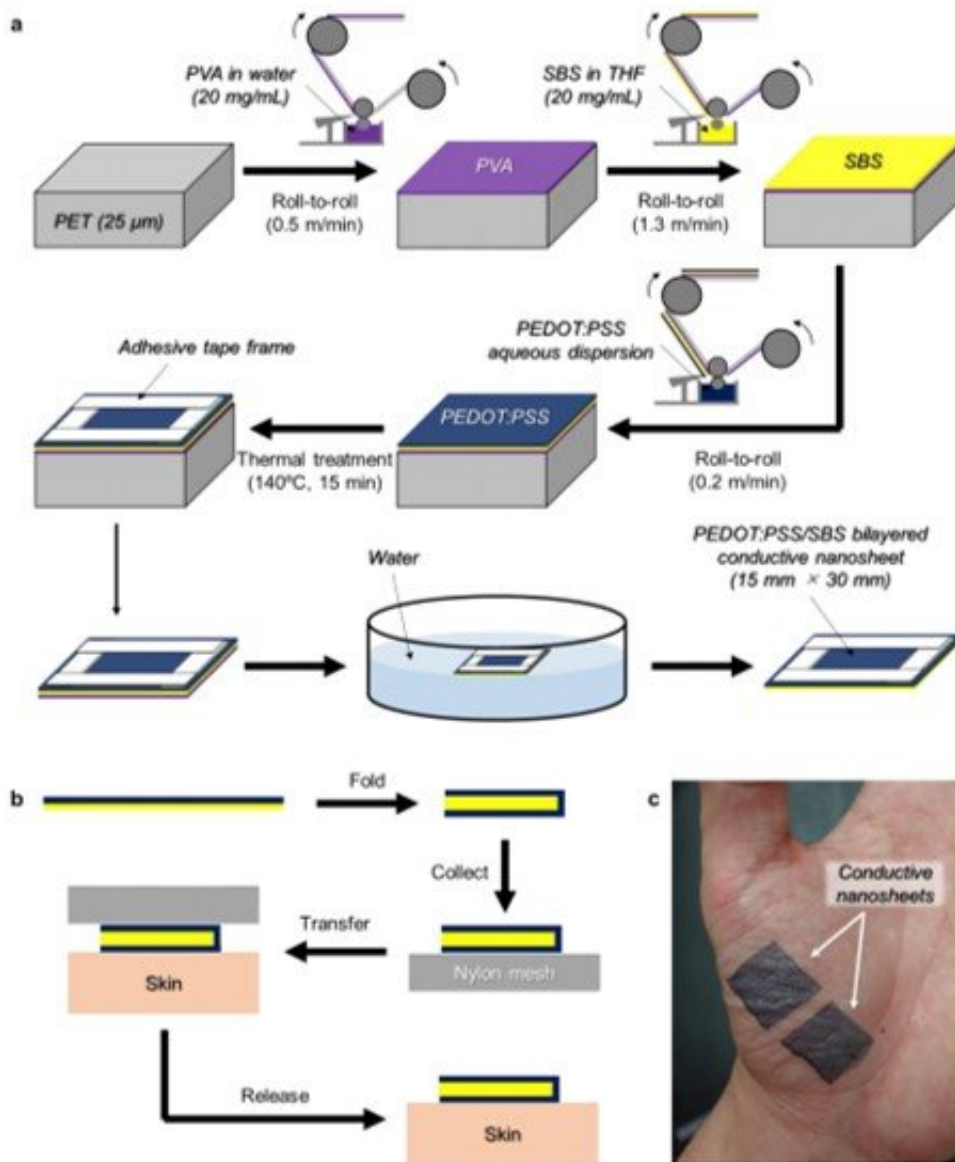

Preparation of conductive polymer nanosheets. (a) Schematic illustration of the fabrication of PEDOT:PSS/SBS bilayered conductive nanosheets by a gravure coating-based roll-to-roll method. A free-standing conductive nanosheet, that was supported by adhesive paper tape frame, was obtained by a water-soluble PVA sacrificial layer method. (b) Schematic illustration of the procedure for attachment of the conductive nanosheet on the skin. (c) Image of two conductive nanosheets on the palm skin. Credit: Nature Asia Materials, doi: 10.1038/s41427-019-0183-1

The researchers assembled the constituents to form a patch-type skin-contact device, which they named the "elastic kirigami patch." They conducted precise measurements of sEMG using the device and obtained signals from the abductor pollicis brevis muscle (APBM) during pitching by experienced baseball players. They synchronized the sEMG signals and acceleration of the arm with sequential photographs of the pitching motion using high-speed cameras.

The device developed by the scientists could measure sEMG signals from the palm in a minimally perceivable manner to the wearer. For this, they used conductive polymer ultrathin films based on [poly\(3,4-ethylene dioxothiophene\): poly\(styrene-sulfonate\)](#) (PEDOT:PSS) known as "[conductive nanosheets](#)" to form the ultraconformable skin-contact electrodes. The team had previously investigated the mechanical and electrical stability of the PEDOT:PSS-based conductive nanosheets against sweat and found them to retain electrical function with structural integrity [after immersion in artificial sweat](#) for 180 minutes. The bilayered elastic conductive nanosheets containing PEDOT:PSS and polystyrene-polybutadiene-polystyrene triblock copolymer (SBS) conformably adhered to [human skin](#) without any adhesive reagents and without interfering with [the natural deformation of skin](#).

The PEDOT:PSS/PBS bilayered conductive nanosheet in the study had a thickness of 339 ± 91 nm, conductivity of 500 S/cm and flexural rigidity less than 10^{-2} nNm (nanonewton meter). The flexibility, stretchability and robust nature of the SBS nanosheet allowed the bilayered conductive nanosheet to conform to skin adhesion via [van-der-Waals forces](#) without adhesive agents. Yamagishi et al. tested the mechanical and elastic stability of the nanosheets on the palm muscle of a subject against repetitive mechanical stretching and contractions. They placed two sheets of Au-sputtered [polyimide](#) thin films on either side of the nanosheet to provide electrical contact with the nanosheets.

Thereafter, they covered the nanosheet and Au-sputtered polyimide thin films with a polyurethane-based transparent adhesive plaster. The researchers measured the resistance of the nanosheet in its initial state and after contraction/stretching of the palm muscle. They did not observe damage even after repetitive cycles of stretching and contractions to clearly demonstrate consistency of the structure and electrical property of the nanosheet electrode, even at maximum strain of the palm. The results suggest their suitability to function as bioelectrodes under repetitive cycles of stretching or contraction. The team constructed and tested the kirigami wiring system to investigate its mechanical and electrical properties and detected the mechanical properties of the wiring system using a tensile tester. The elastic wiring system demonstrated hybrid kirigami-based stretchability and silicone-rubber-based elasticity.

Elastic kirigami patch for electromyographic analysis of the palm muscle during baseball pitching

*Kento Yamagishi, Takenori Nakanishi, Sho Mihara, Masaru Azuma, Shinji Takeoka,
Kazuyuki Kanosue, Tomoyuki Nagami*, Toshinori Fujie**

*Waseda University, Tokyo, Japan
Kitasato University, Kanagawa, Japan
Tokyo Institute of Technology, Kanagawa, Japan
Japan Science and Technology Agency, PRESTO, Saitama, Japan*

Contact: kento-yamagishi@ruri.waseda.jp (K.Y.), t-nagami@kitasato-u.ac.jp (T.N.), t_fujie@bio.titech.ac.jp (T.F.)

Tensile test of the elastic kirigami wiring. Credit: Nature Asia Materials, doi: 10.1038/s41427-019-0183-1

The research team then conducted extensive tests in the lab to understand the insulation property of kirigami wiring and shape recovery after elongation and contraction. To test the skin-contact device optimized with an elastic kirigami patch and a Bluetooth module, they measured electrode-skin contact impedance before and after the participants performed an arm swing. The scientists compared the results with a non-kirigami sample. Using three high-speed cameras, they captured the pitching motion of participants to investigate the SEMG signal pattern between the APBM and other muscles.

Yamagishi et al. then investigated the pitching motion in five separate phases; windup, early cocking, late cocking, acceleration and follow-through. They credited the generally observed difficulty for pitchers to control curveballs (compared with fastballs), to strengthening and weakening of APBM activity, approximately -0.5 seconds after throwing a curveball. The electromyographic analyses of the APBM during pitching motion with the intact elastic kirigami patch indicated that pitchers controlled the palm muscle activity during the early cocking phase prior to releasing the ball.



Pitching motion of participant throwing a curveball. Credit: Nature Asia Materials, doi: 10.1038/s41427-019-0183-1

In this way, Kento Yamagishi and co-workers developed a skin-contact patch device with a kirigami-inspired stretchable wiring system and conductive nanosheet-based ultraconformable bioelectrodes. They successfully conducted dynamic sEMG analyses of the APBM muscle, which could not be tested with conventional devices during baseball pitching. The minimally perceivable device can be used to investigate the activity of muscles of athletes during exercise without interfering with their performance. The sEMG recordings observed in the work will allow researchers to obtain deeper understanding of muscle activity across a wide range of sports and movements.

More information: Kento Yamagishi et al. Elastic kirigami patch for electromyographic analysis of the palm muscle during baseball pitching, *NPG Asia Materials* (2019). [DOI: 10.1038/s41427-019-0183-1](https://doi.org/10.1038/s41427-019-0183-1)

D.-H. Kim et al. Epidermal Electronics, *Science* (2011). [DOI: 10.1126/science.1206157](https://doi.org/10.1126/science.1206157)

Melina K. Blees et al. Graphene kirigami, *Nature* (2015). [DOI: 10.1038/nature14588](https://doi.org/10.1038/nature14588)

© 2019 Science X Network

Citation: Elastic kirigami patch for electromyographic analysis of the palm muscle during baseball pitching (2019, December 27) retrieved 24 April 2024 from <https://phys.org/news/2019-12-elastic-kirigami-patch-electromyographic-analysis.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.