


# The invention of a flexible endoscope thinner than a needle

September 5 2022

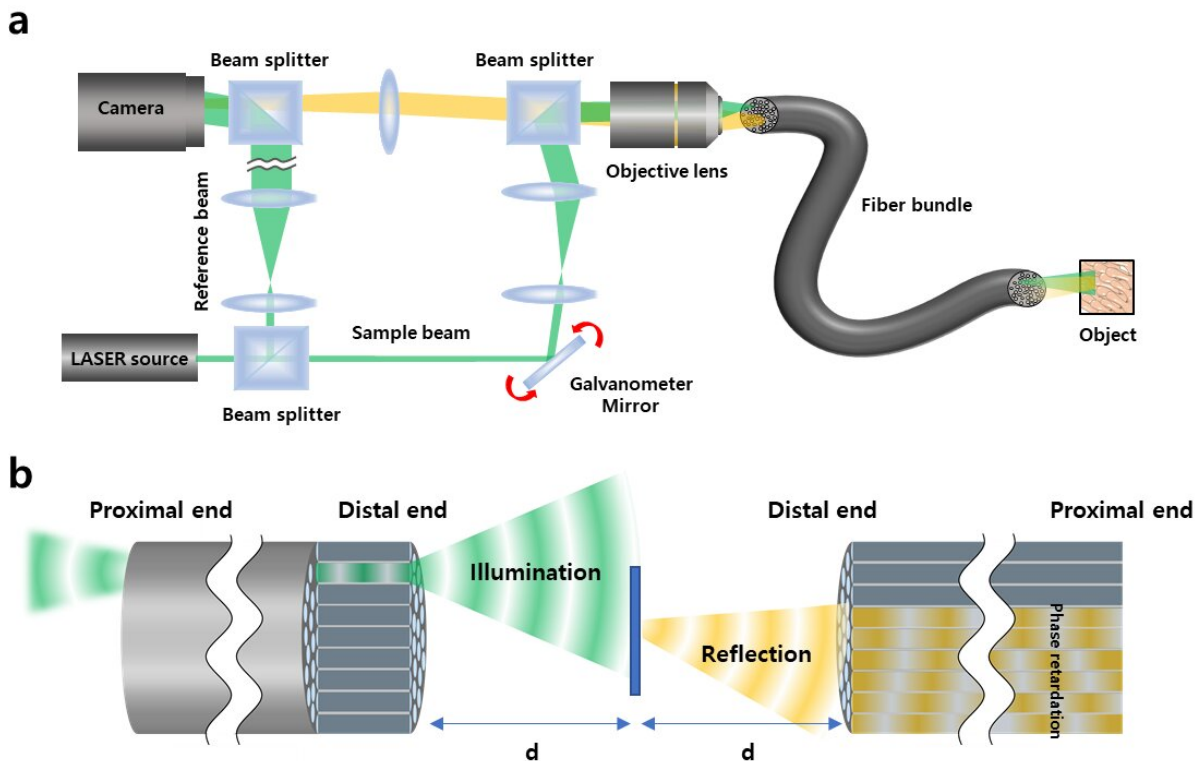


Experimental setup of ultrathin holographic endomicroscope. (a) The output beam from a laser is divided into sample and reference beams. The sample beam is delivered to the sample through the fiber bundle. The backscattering signal from the sample, indicated as yellow for clarity although its wavelength is identical to the incident wave, is captured by the fiber bundle and delivered to the camera. The reference beam generates an interferogram together with the signal beam at the camera. (b) Image formation principle. The angular spectrum of the sample is obtained under Fresnel conditions by separating the distance

between the object and the optical fiber. Credit: Institute for Basic Science

If you are used to getting regular health checkups, you might be familiar with endoscopes. The endoscope is an imaging device consisting of a camera and a light guide attached to a long flexible tube. It is particularly useful for acquiring images of the inside of a human body. For example, stomach and colon endoscopy are widely used for the early detection and diagnosis of diseases such as ulcers and cancers.

In general, an endoscope is manufactured by attaching a camera sensor to the end of a probe or using an optical fiber, which allows for information to be transmitted using light. In the case of an endoscope that uses a camera sensor, the thickness of the probe increases, which makes the endoscopy rather invasive. In the case of an endoscope using an optical fiber bundle, it can be manufactured in a thinner form factor, which minimizes invasiveness and results in much less discomfort to the patients.

However, the downside is that in a conventional fiber-bundle endoscope, it is difficult to perform [high-resolution imaging](#), because the resolution of the obtained image is limited by the size of the individual fiber cores. Much of the image information is also lost due to reflection from the probe tip. Furthermore, in fiber endoscopy, it is often necessary to label the target with fluorescence, especially in [biological samples](#) with low reflectivity, due to strong back-reflection noise generated from the tip of the thin probe.

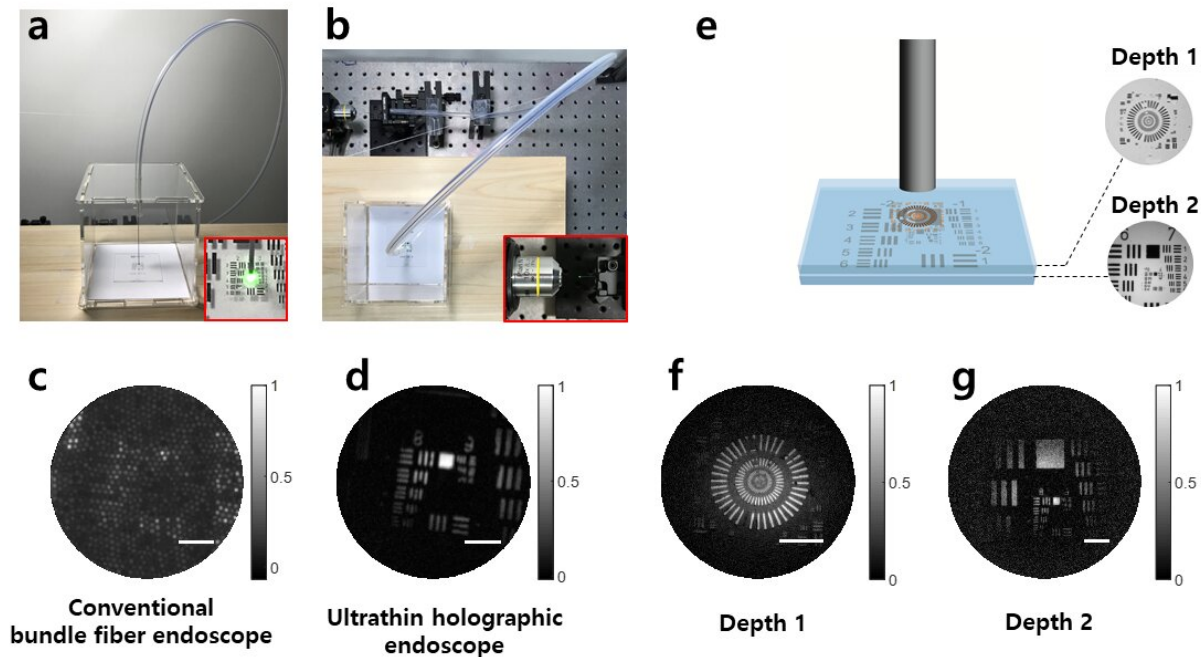


Endoscopic imaging through a narrow and curved passage, and 3D imaging capability. (a) and (b) show front and top views of the experimental configuration, respectively. (c) and (d) show the conventional endoscopic image and the reconstructed image with the newly developed endoscope, respectively. Scale bars: 20  $\mu\text{m}$ . (e) shows endoscopic imaging of stacked targets. Two resolution targets were placed at two different depths, 1 and 2. Ground-truth images of the targets in depths 1 and 2 taken by conventional brightfield microscope were shown next to the schematic. (f) and (g) display endoscopic images for the depths of 1 and 2, respectively, reconstructed using a single reflection matrix recording. Credit: Institute for Basic Science

Recently, a research team led by CHOI Wonshik, the Associate Director of the Center for Molecular Spectroscopy and Dynamics (CMSD) within the Institute for Basic Science (IBS), has developed a high-resolution holographic endoscope system. The researchers were able to overcome the previous limitation of fiber optic endoscopy and were able to reconstruct high-resolution images, without attaching a lens or any

equipment to the distal end of the fiber bundle.

This feat was accomplished by measuring the holographic images of the light waves that are reflected from the object and captured by the fiber bundle. The researchers first illuminated an object by focusing light onto a single core of a fiber bundle and measured holographic images that were reflected from the object at a certain distance from the optical fiber. In the process of analyzing the holographic images, it was possible to reconstruct the object image with a microscopic resolution by correcting the phase retardation that occurs by each fiber core. Specifically, a unique coherent image optimization algorithm was developed to eliminate fiber-induced phase retardations in both the illumination and detection pathways and reconstruct an object image with a microscopic resolution.

Since the developed endoscope does not attach any equipment to the end of the optical fiber, the diameter of the endoscope probe is 350  $\mu\text{m}$ , which is thinner than the needle used for hypodermic injection. Using this approach, researchers were able to obtain high-resolution images with a spatial resolution of 850 nm, which is far smaller than the core size of the [optical fiber](#) bundle.

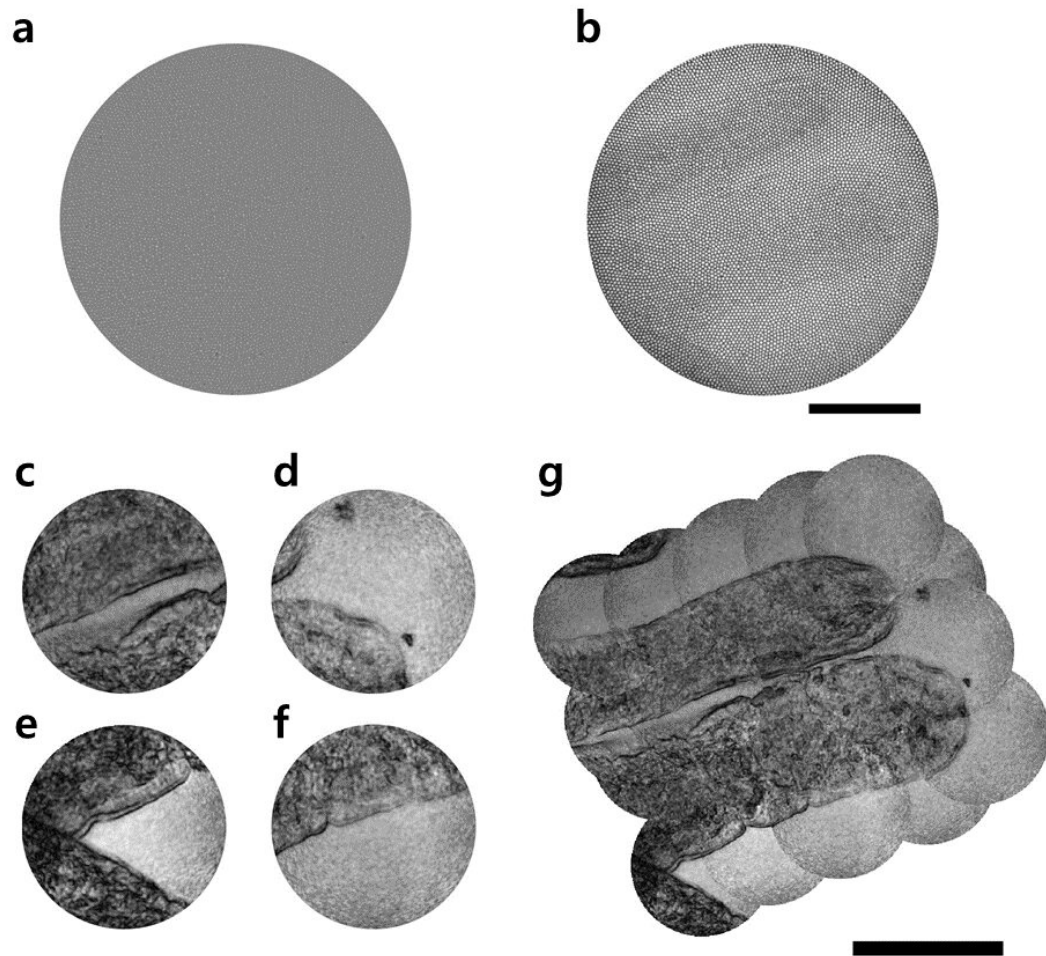

Microscopic imaging of villi in a rat intestine. (a) shows conventional reflectance endoscope image taken when the fiber bundle was in contact with the villi. (b) shows transmission image obtained through the fiber bundle. The LED illumination was sent from the villi to the fiber bundle. (c)-(f) display label-free reflectance images obtained using the newly developed holographic endoscope. (g) shows a reconstructed image of two villi by stitching multiple images taken over a wide region of interest. The 350- $\mu\text{m}$ -diameter fiber bundle was used for image acquisition. Scale bar: 100  $\mu\text{m}$ . Credit: Institute for Basic Science

The researchers went on to test the new Fourier holographic endoscopy system to image the villi structure of mice. It was possible to acquire high contrast image by effectively removing the back-reflection noise of the probe, even in biological samples with very low reflectivity, such as rat villi. In addition, post-processing of the measured holographic information made it possible to reconstruct multi-depth 3D images from a single data set with a depth resolution of 14  $\mu\text{m}$ .

It is believed that the practical application of this new endoscope will greatly improve the way we can image the internal structures of our body in a minimally invasive manner, with little to no discomfort for patients. It will also open the possibility of directly observing cavities as small as microvessels and the smallest airways in the lungs, which was impossible with preexisting technologies. The researchers even suggested the application of their new endoscope can go well beyond the [medical field](#), as it can potentially be useful for industrial inspections of semiconductors and microprocessors.

The research was published in *Nature Communications*.

**More information:** Wonjun Choi et al, Flexible-type ultrathin holographic endoscope for microscopic imaging of unstained biological tissues, *Nature Communications* (2022). [DOI: 10.1038/s41467-022-32114-5](#)

Provided by Institute for Basic Science

Citation: The invention of a flexible endoscope thinner than a needle (2022, September 5) retrieved 16 June 2024 from <https://phys.org/news/2022-09-flexible-endoscope-thinner-needle.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.