


# New electromagnetic device could catapult mechanobiology research advances into the clinical arena

January 18 2023

---

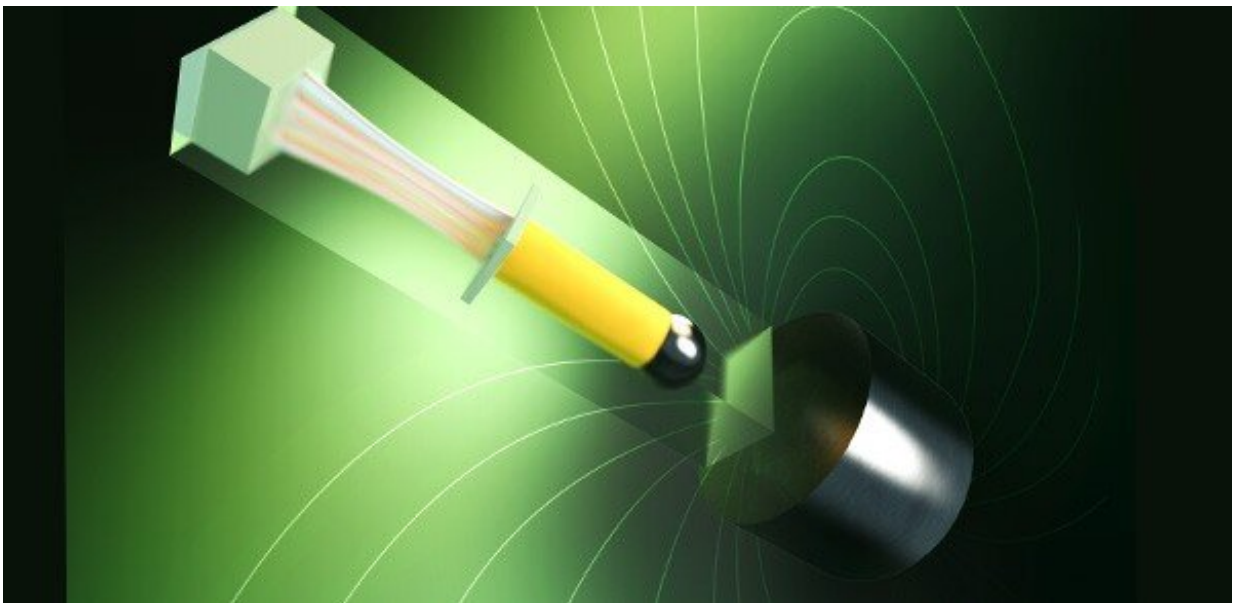

An artist's impression of the new electromagnetic device showing a tissue specimen being tested under tension using the attraction between a steel ball and an electromagnet. Credit: BioHues Digital

A new electromagnetic device that enables high-precision measurements of a broad range of soft biological tissues, has established a new standard of precision in the mechanobiology field, say researchers. The method allows for the mechanical testing of tissues the size of human biopsy

samples, making it particularly relevant for studies of human disease.

The body's soft tissues exhibit a wide range of mechanical properties, such as stiffness and strength, which are critical to carry out their function. For example, the tissues of the gastrointestinal tract are soft to allow for the transit and digestion of food, whereas tendons are relatively more stiff to transmit force from muscle to bone allowing us to move.

The ability to accurately measure the mechanical properties of these tissues, which are subject to change during developmental processes or because of disease, has profound implications for the fields of biology and medicine. Methods to measure these properties are currently inadequate, and their accuracy and reliability remains limited—until now.

New research involving researchers from the University of Cambridge and the MIT Institute for Medical Engineering and Science (IMES) has resulted in a device that relies on magnetic actuation and optical sensing, thus potentially allowing for live imaging of the [tissue](#) under an inverted microscope. This way, insights can be gained into the behavior of the tissue under mechanical forces at both a cellular and [molecular level](#). The results are reported in the journal *Science Advances*.

An electromagnet exerts a pulling force on the tissue specimen which is mounted on the device, while an optical system measures the specimen's change in size or shape.

"One of the most critical requirements for mechanical testing of soft biological tissues is the need to mimic the biological specimen's physiological conditions (e.g., temperature, nutrients) as closely as possible, in order to keep the tissue alive and preserve its biomechanical properties," said Dr. Thierry Savin, Associate Professor in Bioengineering, who led the research team.

"To this end, we designed a transparent mounting chamber to measure the mechanical properties of tissues—at the millimeter scale—in their native physiologic and chemical environment. The result is a more versatile, precise and robust device that shows high reliability and reproducibility."

To directly assess the performance of their electromagnetic device, the researchers conducted a study on the biomechanics of a mouse esophagus and of its constitutive layers. The esophagus is the muscular tube connecting the throat with the stomach and it is composed of multiple tissue layers. The researchers used the device to conduct the first biomechanical investigation of each of the three individual layers of the mouse esophageal tissue.

Their findings showed that the esophagus behaves like a three-layer composite material akin to those commonly used in several engineering applications. To the researchers' knowledge, these are the first results acquired of the mechanical properties of each individual layer of the esophagus.

"Our study demonstrated the enhanced reliability of the electromagnetic device, yielding errors in the stress-strain response below 15%—a level of accuracy not seen before," said Dr. Adrien Hallou, Postdoctoral Fellow at the Wellcome Trust/Cancer Research UK Gurdon Institute. "We hope that this device may eventually become the new standard in the tissue biomechanics field, providing a standardized dataset for the characterization of mouse and human soft tissue mechanics across the board."

Luca Rosalia, Ph.D. candidate at IMES, added, "Through analysis of the biomechanics of healthy tissues and their changes as they occur during disease, our device could eventually be used to identify alterations in tissue properties that are of diagnostic relevance, therefore becoming a

valuable tool to inform clinical decisions."

**More information:** Luca Rosalia et al, A magnetically actuated, optically sensed tensile testing method for mechanical characterization of soft biological tissues, *Science Advances* (2023). [DOI: 10.1126/sciadv.ade2522](https://doi.org/10.1126/sciadv.ade2522)

Provided by University of Cambridge

Citation: New electromagnetic device could catapult mechanobiology research advances into the clinical arena (2023, January 18) retrieved 26 April 2024 from <https://phys.org/news/2023-01-electromagnetic-device-catapult-mechanobiology-advances.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.