


Scientists propose novel NO₂ sensor based on static magnetic field Faraday rotation spectroscopy

January 30 2023, by Zhang Nannan

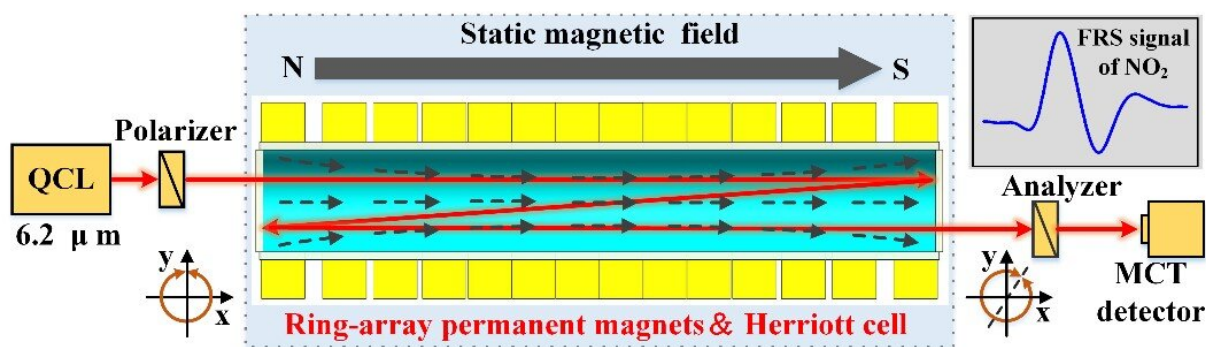

Schematic diagram of static magnetic field FRS NO₂ sensor. Credit: Cao Yuan


A low-power Faraday rotation spectroscopy (FRS) nitrogen dioxide (NO₂) sensor basing on ring array permanent magnets was proposed by researchers led by Prof. Gao Xiaoming from the Hefei Institutes of Physical Science of the Chinese Academy of Sciences (CAS), according to a study published in *Analytical Chemistry*.

FRS enables detection of paramagnetic molecules by detecting changes in the polarization state of linearly polarized light caused by a gaseous medium immersed in an external longitudinal magnetic field. It is not disturbed by diamagnetic molecules such as CO₂ and H₂O, so it exhibits


a high species specificity. In addition, it has very high detection sensitivity due to the use of a pair of nearly-crossed polarizers that greatly suppress laser intensity noise.

The current FRS signal is mainly generated by the Zeeman splitting of the sample absorption lines modulated by an alternating magnetic field generated by a solenoid coil. However, when exciting the magneto-optical effect, this sinusoidal electromagnetic field suffers from high power consumption, generation of large amounts of Joule heat, [electromagnetic interference](#), etc.

To solve these problems, the researchers proposed a static magnetic field FRS sensing device based on rare-earth [permanent magnets](#).

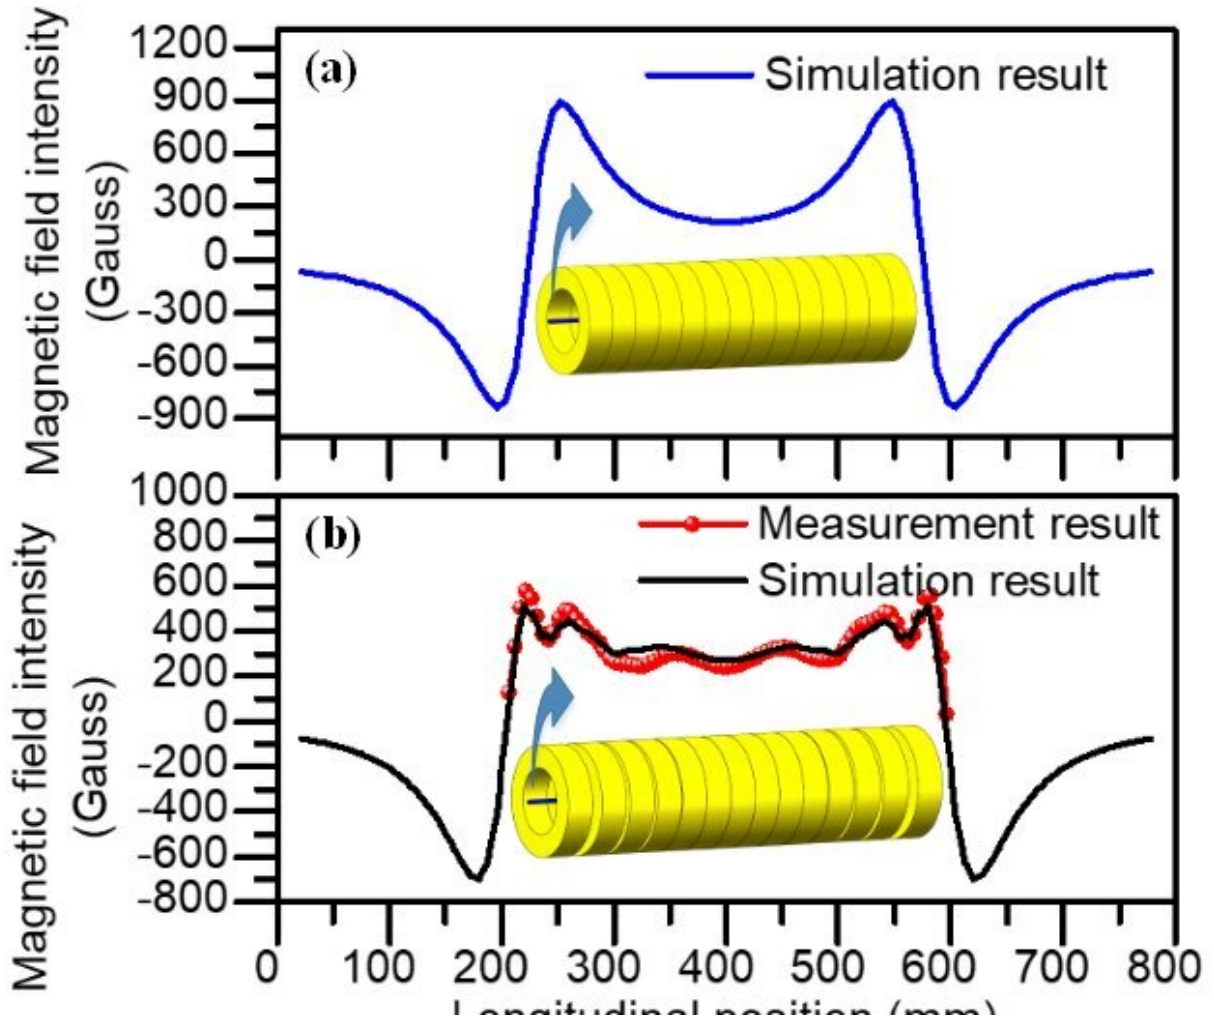

Schematic diagram of NdFeB permanent magnet ring array and its magnetic field distribution characteristics. Credit: Cao Yuan

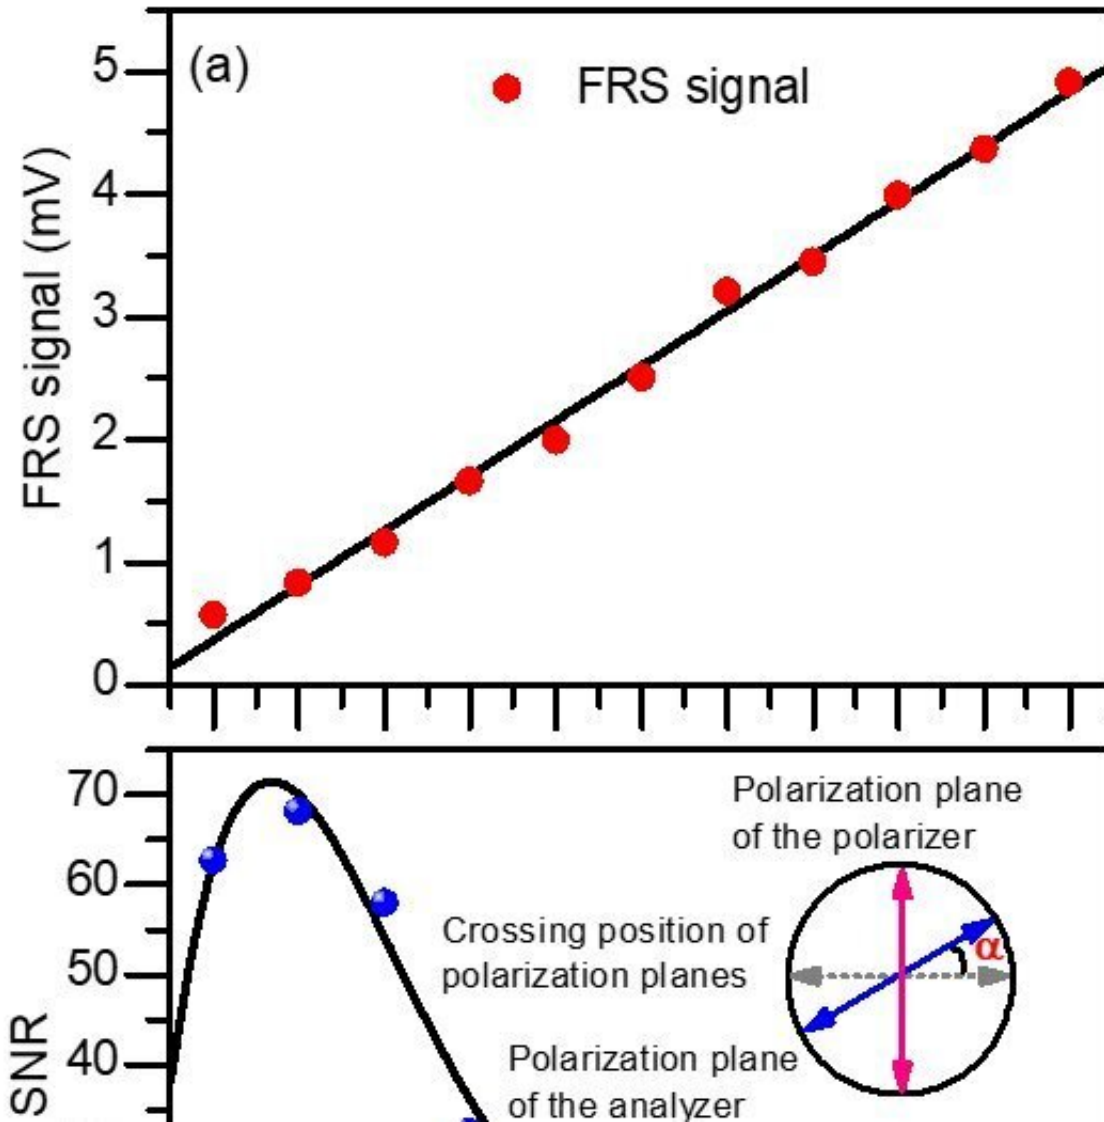

FRS signal and signal-to-noise ratio as a function of the analyzer angle α . Credit: Cao Yuan

According to the magnetic field distribution characteristics of neodymium-iron-boron (NdFeB) permanent magnet rings, they combined 14 identical NdFeB permanent magnet rings in the form of non-equidistance, and obtained a static magnetic field with an average magnetic field intensity of 346 gauss over a length of 380 mm. The interaction between linearly polarized light and the sample was greatly

enhanced by fitting the Herriott cell coaxially to the permanent magnet array.

A Q-branch spectral feature in the ν_3 fundamental band of NO_2 at $1,613.25 \text{ cm}^{-1}$ was probed by a mid-infrared quantum cascade laser. The NO_2 detection limit of 0.4 ppb was achieved at an optical length of 23.7 m.

"We expect it to be developed into a robust field-deployable environment monitoring system," said Cao Yuan, first author of the study.

More information: Yuan Cao et al, NO_2 Sensor Based on Faraday Rotation Spectroscopy Using Ring Array Permanent Magnets, *Analytical Chemistry* (2023). [DOI: 10.1021/acs.analchem.2c04821](https://doi.org/10.1021/acs.analchem.2c04821)

Provided by Chinese Academy of Sciences

Citation: Scientists propose novel NO_2 sensor based on static magnetic field Faraday rotation spectroscopy (2023, January 30) retrieved 26 April 2024 from <https://phys.org/news/2023-01-scientists-no2-sensor-based-static.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.