


Research team demonstrates a new 'primary standard' for measuring ultralow pressures

August 10 2023

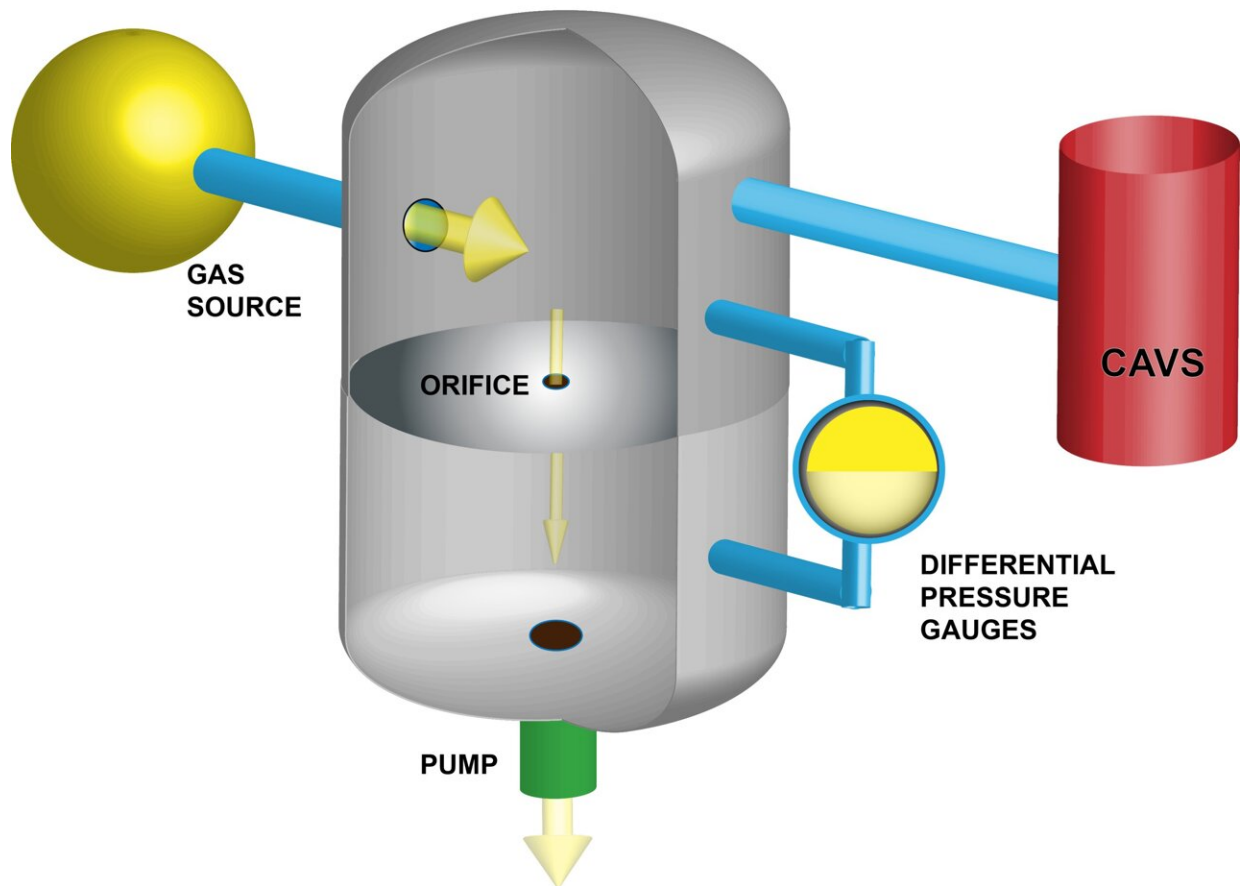

To verify the accuracy of their new approach for measuring ultra-low vacuum pressures, NIST researchers built a high-performance version of a traditional pressure metrology setup, known as a dynamic expansion system. In this system, they injected gas at a flow rate of roughly 10 to 100 billion molecules per second into the top chamber. The gas moved from the upper chamber to the lower

chamber, which is evacuated by a large pump, at a known rate through a precisely dimensioned orifice. A set of gauges measured the pressure ratio between the top and bottom chambers to correct for imperfections. Using the flow rate of gas in and the rate that gas moves from between the two chambers, the researchers calculated the pressure in the top chamber, which the CAVS independently measures. The researchers found agreement between this known pressure value and the readings from the CAVS sensors, thereby validating their new method. Credit: NIST

A vacuum chamber is never perfectly empty. A small number of atoms or molecules always remain, and measuring the tiny pressures they exert is critical. For instance, semiconductor manufacturers create microchips in vacuum chambers that must be almost entirely devoid of atomic and molecular contaminants, and so they need to monitor the gas pressure in the chamber to ensure that the contaminant levels are acceptably low.

Now, scientists at the National Institute of Standards and Technology (NIST) have validated a new approach to measuring extremely low gas pressures called CAVS, for cold atom vacuum standard. They have established that their technique can serve as a "primary standard"—in other words, it can make intrinsically [accurate measurements](#) without first needing to be calibrated to reference [pressure](#) readings.

Having developed CAVS over the last seven years, NIST researchers recently put their technique through its most rigorous tests to date. Their new study, in the journal *AVS Quantum Science*, shows that CAVS results agreed with the traditional "gold standard" method for measuring low pressures, demonstrating that this new technique can make measurements with the same degree of accuracy and reliability.

Not only can CAVS make measurements as good as those in traditional pressure gauges, but it can also reliably measure the much lower vacuum


pressures—a trillionth of the Earth's sea-level atmospheric pressure and below—that will be required for future chip manufacturing and next-generation science. And its operation, based on well-understood quantum physics principles, means that it can make accurate readings "right out of the box," without requiring any adjustments or calibration to other reference pressure sources or techniques.

"This is the culminating result," said NIST physicist Julia Scherschligt. "We have had numerous positive developments before. But this validates the fact that our cold atom standard is truly a standard."

In addition to semiconductor manufacturing, the new method can be useful for other applications that require high-vacuum environments, such as quantum computers, [gravitational wave detectors](#), particle accelerators and many more.

CAVS technology measures vacuum pressures using a cold gas of about a hundred thousand lithium or rubidium atoms trapped in a magnetic field. These atoms fluoresce when illuminated by a laser tuned to just the right frequency. Researchers can count the number of trapped atoms precisely by measuring the intensity of this glow.

When the CAVS sensor is connected to a vacuum chamber, the leftover atoms or molecules in the chamber collide with the trapped atoms. Each collision knocks an atom out of the trap, reducing the number of atoms and the intensity of light emitted. That intensity, easily measured by light sensors, serves as a sensitive measure of pressure. This relationship between the rate of dimming and the number of molecules is predicted exactly by quantum mechanics.

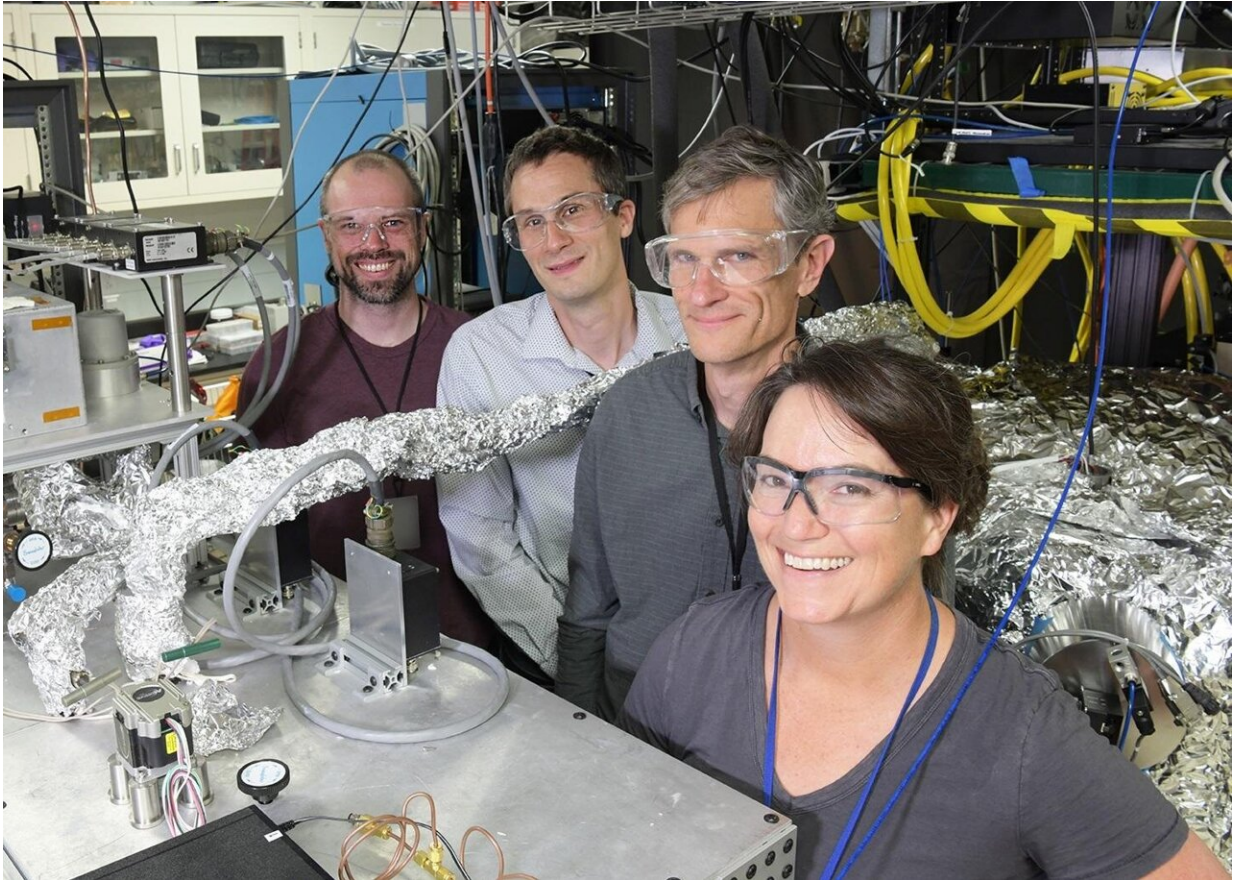

NIST researchers Dan Barker, Steve Eckel, Jim Fedchak, Julia Scherschligt and their colleagues developed and tested a new method, known as the cold atom vacuum standard (CAVS), for measuring ultralow pressures. Credit: NIST

In the new work, the NIST researchers attached their CAVS sensors to the classical gold-standard reference standard for gas pressure, known as a dynamic expansion system.

Dynamic expansion systems work by injecting a known amount of gas, measured in molecules per second, into a [vacuum chamber](#), then slowly removing the gas from the other end of the chamber at a known rate. The researchers then calculate the resulting pressure in the chamber.

In this experiment, the researchers built a high-performance dynamic expansion system that allowed for extremely small flows of gas—in the range of 10 billion to 100 billion atoms or molecules per second—and included a custom-built flowmeter to measure flows that low. The hole they built to remove atoms slowly from the [chamber](#) was machined to submicrometer precision.

"The heavy lifting needed to stand up one of these classical standard devices is monumental," Scherschligt said. "Going through the effort of doing that really drove home the point of this whole experiment, which is that CAVS provides high accuracy in a much simpler form."

The NIST researchers tested two types of CAVS sensors in their work. One is a laboratory version; the second is a mobile version that can easily be used in advanced chip manufacturing settings.

"Indeed, the portable version is so simple, we eventually decided to automate it such that we very rarely had to intervene in its operation. In fact, most of the data from the portable CAVS for this study was taken while we were comfortably asleep at home," said NIST physicist Dan Barker.

"The gases we measured—including nitrogen, helium, argon and even neon—are all inert semiconductor process gases," said NIST physicist Steve Eckel. "But in the future, we hope to measure more reactive gases like hydrogen, [carbon dioxide](#), carbon monoxide and oxygen, which are all both common residual gases found in vacuum chambers and useful gases for semiconductor manufacturing."

Together, these CAVS systems promise to help researchers working with ultralow pressures reach new highs in both science and technology.

More information: Daniel S. Barker et al, Accurate measurement of

the loss rate of cold atoms due to background gas collisions for the quantum-based cold atom vacuum standard, *AVS Quantum Science* (2023). [DOI: 10.1116/5.0147686](https://doi.org/10.1116/5.0147686)

Provided by National Institute of Standards and Technology

Citation: Research team demonstrates a new 'primary standard' for measuring ultralow pressures (2023, August 10) retrieved 29 April 2024 from <https://phys.org/news/2023-08-team-primary-standard-ultralow-pressures.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.