


# Researchers develop perovskite X-ray detector for medical imaging

May 21 2024

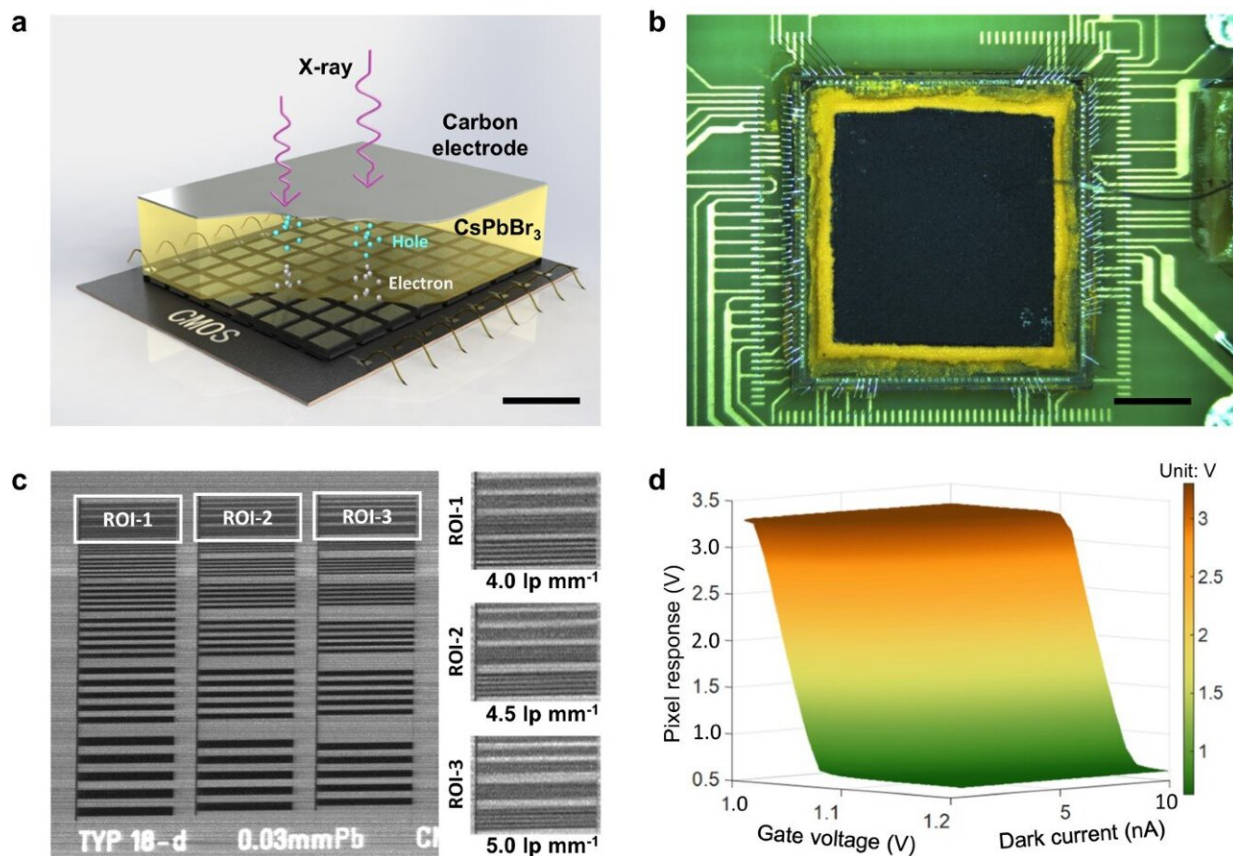

Inorganic CsPbBr<sub>3</sub> based direct-conversion X-ray CMOS detector. Credit: SIAT / Yongshuai Ge

Shenzhen Institutes of Advanced Technology (SIAT) of the Chinese Academy of Sciences, in collaboration with researchers at Central China

Normal University, have developed a high-performance perovskite X-ray complementary metal-oxide-semiconductor (CMOS) detector for medical imaging.

The [study was published](#) in *Nature Communications* on Feb. 21.

X-ray imaging is vital for the diagnosis and treatment of cardiovascular and cancer diseases. Direct-conversion X-ray detectors made of semiconductor materials exhibit superior spatial and [temporal resolution](#) at lower radiation doses compared to indirect-conversion detectors made of scintillator materials. However, the currently available semiconductor materials, such as Si, a-Se, and CdZnTe/CdTe, are not ideal for general X-ray imaging due to their low X-ray absorption efficiency or [high costs](#).

Perovskite is a promising alternative to conventional [semiconductor materials](#). However, the feasibility of its combination with high-speed pixelated CMOS arrays is still unknown.

To address this issue, researchers developed a direct-conversion X-ray detector fabricated with a 300  $\mu\text{m}$  thick inorganic CsPbBr<sub>3</sub> perovskite film printed on a dedicated CMOS pixel array.

Researchers found that the screen-printed thick CsPbBr<sub>3</sub> film has a high  $\mu\tau$  product of  $5.2 \times 10^{-4} \text{ cm}^2 \text{ V}^{-1}$ , a high X-ray detection sensitivity of  $15,891 \mu\text{C Gy}_{\text{air}}^{-1} \text{ cm}^{-2}$ , and a low dose detection limit of  $321 \text{ nGy}_{\text{air}} \text{ s}^{-1}$ .

Experimental X-ray 2D imaging results showed that the proposed perovskite CMOS detector can achieve very [high spatial resolution](#) (5.0 lp mm<sup>-1</sup>, hardware limit is 6.0 lp mm<sup>-1</sup>) and low-dose (260 nGy) imaging performance.

Moreover, 3D CT imaging was also validated with the proposed detector at a fast signal readout speed of 300 fps.

"Our work shows the potential of lead halide perovskites in revolutionizing the development of state-of-the-art X-ray detectors with significantly enhanced spatial resolution, readout speed, and low-dose detection efficiency," said Prof. Ge.

"This paves the road for medical X-ray imaging applications to become gentler and safer in the future."

**More information:** Yanliang Liu et al, Dynamic X-ray imaging with screen-printed perovskite CMOS array, *Nature Communications* (2024). DOI: [10.1038/s41467-024-45871-2](https://doi.org/10.1038/s41467-024-45871-2)

Provided by Chinese Academy of Sciences

Citation: Researchers develop perovskite X-ray detector for medical imaging (2024, May 21) retrieved 13 July 2024 from <https://phys.org/news/2024-05-perovskite-ray-detector-medical-imaging.html>

This document is subject to copyright. Apart from any fair dealing for the purpose of private study or research, no part may be reproduced without the written permission. The content is provided for information purposes only.